


FLOW SPLITTER, FOR OXYGEN CONCENTRATOR

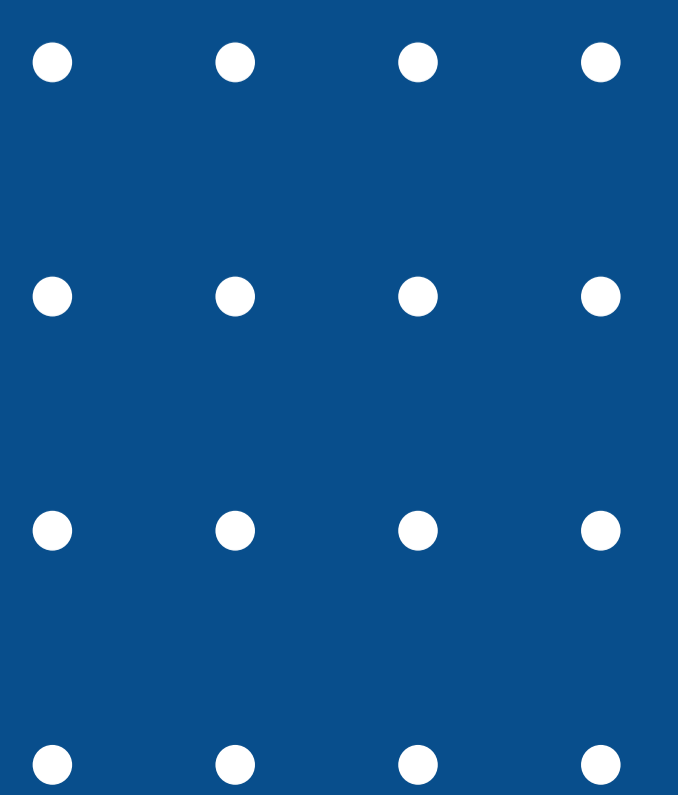

Flow splitter, for oxygen concentrator

TECHNICAL SPECIFICATION:

- Equipped with five independent, Thorpe tube flow meters, to measure and regulate the flow of medical gas.
- Suitable for cleaning and disinfection with hospital-grade cleaning products.
- Inlet port is DISS format.
- 6 mm barbed outlets.
- Flow meter columns are transparent, clearly readable and graduated (metric system).
- Inlet pressure up to at least 20 psi (138 kPa).
- 0-2 L/min, accuracy better than 10%, graduation 0.125 L/min or lower.

ITEMS REQUIRED, BUT NOT SUPPLIED:

- Oxygen Concentrator
- Humidifier
- Nasal prongs

ENVIRONMENTAL CONDITIONS

- Operating conditions: 5 to 40° C, relative humidity 15 to 90% non-condensing.
- Storage conditions: 5 to 50° C, relative humidity 15 to 90% non-condensing.

WARRANTY:

24 months

REGULATION & CONFORMITY REQUIREMENTS

Accessory to oxygen concentrator with CE mark conforming to Medical Device Directive 93/42/EEC

Accessory to oxygen concentrator with CE Certificate (class IIa)